

ELISA Flex: Human Latent TGF- β 1 (ALP)

3550-1A-6 | 3550-1A-20

ELISA Flex kit for quantitative determination of native and recombinant human latent Transforming Growth Factor- β 1 (TGF- β 1) in solution, e.g. cell supernatant.

The kit includes		3550-1A-6 for 6 plates	3550-1A-20 for 20 plates
Capture mAb:	MT593 (0.5 mg/ml)	300 μ l	1000 μ l
Detection mAb:	MT517, biotin (0.5 mg/ml)	150 μ l	500 μ l
Streptavidin-ALP		80 μ l	250 μ l
Recombinant human LAP (homodimer) ELISA standard		1 vial	1 vial
Standard reconstitution buffer A8		1 ml	1 ml

To ensure total recovery of the stated quantity, vials have been overfilled.

Shipping and storage

Shipped at ambient temperature. All reagents should be stored at 4-8 °C upon receipt, except the standard which should be stored at -20 °C. Antibodies are supplied in sterile-filtered PBS with sodium azide (0.02%). Streptavidin-ALP is supplied in 0.1 M Tris buffer with 0.002% Kathon CG. The expiry date indicates how long unopened products, stored according to instructions, are recommended for use.

General and Preparations

Specificity

The kit contains a matched pair of monoclonal antibodies (mAbs) specific for LAP entity of human latent TGF- β 1. This enables direct quantification of latent TGF- β 1 in ELISA with no need of sample pre-treatment. The ELISA does not detect human latent TGF- β 2 or - β 3 or bovine latent TGF- β 1. The mAbs in this kit cross-react with latent TGF- β 1 from non-human primates. Please visit www.mabtech.com for reactivity on NHP species.

Standard range

0.5-50 pM

Calibration


Since the included LAP standard differs in molecular weight from latent TGF- β 1, determination of latent TGF- β 1 using the standard curve is based on a molar comparison. 1 pM LAP corresponds to 1 pM latent TGF- β 1. For conversion from pM to pg/ml: 1 pM LAP = 54 pg/ml and 1 pM latent TGF- β 1 = 80 pg/ml.

Analysis of serum and plasma samples

Minimize platelet content in plasma by an additional centrifugation at 10,000 x g for 10 min in connection with the plasma preparation. Analysis of serum/plasma requires the use of ELISA diluent (product code: 3652-D2). The ELISA diluent blocks heterophilic antibodies, commonly found in serum/plasma, from cross-linking the assay antibodies, thereby preventing false positive read-outs. The ELISA diluent should be used for dilution of standard, samples, and detection antibody.

Reconstitution of ELISA standard

Reconstitute the standard to a stock solution of 20 nM by adding 1 ml of the standard reconstitution buffer. Allow the standard to dissolve for 5 minutes and mix thoroughly. The standard should be kept in aliquots at -20 °C. Avoid repeated freeze-thaw cycles. Prepare the standard curve within 30 minutes of use.

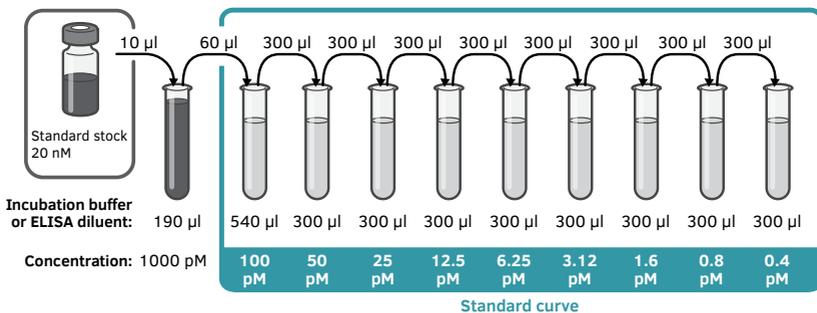


Protocol

Day 1

1. Add 100 μl /well of capture mAb MT593 diluted to 2 $\mu\text{g}/\text{ml}$ in PBS, pH 7.4. Use high protein binding ELISA plates. Incubate overnight at 4-8 $^{\circ}\text{C}$.

Day 2

2. Empty the plate and add 200 μl /well of PBS with 0.05% Tween 20 and 0.1% BSA (incubation buffer) to block the plate. Incubate for 1 hour at room temperature.
3. Wash the plate 5 times with PBS containing 0.05% Tween 20 (300 μl /well).
4. Add 100 μl /well of samples or standards diluted in incubation buffer or ELISA diluent. Include assay background control, i.e. wells without standard. Incubate for 2 hours at room temperature.
5. Wash as above.
6. Add 100 μl /well of detection mAb MT517-biotin diluted to 1 $\mu\text{g}/\text{ml}$ in incubation buffer or ELISA diluent. Incubate for 1 hour at room temperature.
7. Wash as above.
8. Add 100 μl /well of Streptavidin-ALP diluted 1:1000 in incubation buffer. Incubate for 1 hour at room temperature.
9. Wash as above.
10. Add 100 μl /well of pNPP substrate (product code: 3652-P10) and incubate at room temperature protected from direct light for approximately 60 minutes.
11. Measure the optical density in an ELISA reader at 405 nm. Preferably use a reader capable of subtracting a reference wavelength of between 570 and 650 nm. Representative standard curve shown below.

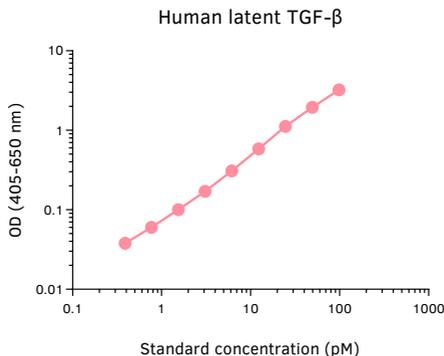

Developed and manufactured by MABTECH AB, Sweden, whose quality management system complies with the standards ISO 9001:2015 & ISO 13485:2016.



The products are for research use only.

MABTECH shall not be liable for the use or handling of the product or for consequential, special, indirect or incidental damages there from.

Mabtech AB (Head Office)
Sweden
Tel: +46 8 716 27 00
mabtech@mabtech.com

Mabtech, Inc.
USA
Tel: +1 513 871-4500
mabtech.usa@mabtech.com